



## Technical Note 120

### SmartPath® and High Absorbance

#### Introduction

DeNovix DS-11 Series instruments utilize proprietary SmartPath® Technology, in conjunction with its innovative microvolume design (Patent US 9442009), to enable measurements of samples with absorbance values as high as 750 AU (at a 1cm equivalent pathlength). This means that bovine serum albumin (BSA) samples up to 1125 mg/mL and dsDNA samples up to 37,500 ng/μL can be accurately and reproducibly quantified using the DS-11.

This technical note will provide some background on the relationship between two terms—transmittance and absorbance—and explain the Beer-Lambert Law. This information will then be used to explain how the DS-11 enables the measurement of samples with ultra high concentrations.


#### Transmittance

Transmittance (T) is defined as the fraction of incident light (radiant power) at a specified wavelength that passes through a sample as represented by Equation 1.

$$\text{eq 1: } T = (I/I_0)$$

$I$  is the light intensity after it passes through the sample, and  $I_0$  is the initial light intensity.

For example, completely transparent samples will have  $I = I_0$ , and therefore the percent transmittance will be 100%. Samples that permit no light at a specified wavelength to pass through will have a percent transmittance of 0%.

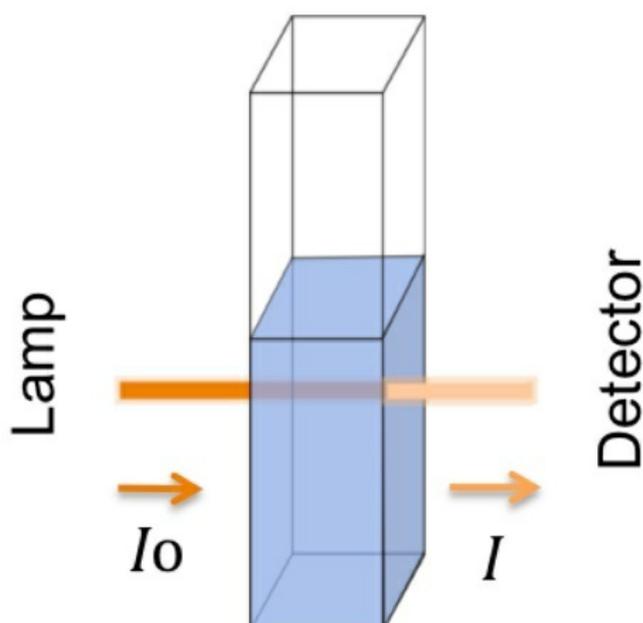

## Absorbance

---

Absorbance (A) is defined as the the capacity of a sample to absorb light (radiation) and is expressed as

the negative log ratio of transmittance (T), as shown in Equation 2.

$$\text{eq 2: } A = -\log T \quad \text{or } A = -\log (I/I_0)$$

**Note:** The  $I/I_0$  in Equation 1 refers to light passed through a single sample. The  $I/I_0$  in Equation 2 refers to light transmitted through a sample as a ratio of the light transmitted through the blank solution.

In Equation 2, if  $A = 0$ , then no photons are absorbed and  $T = 100\%$ . If  $A = 1.00$ , then 90% of the photons are absorbed and 10% reaching the detector ( $T = 10\%$ ).

A practical upper absorbance limit for most spectrometers is 1.5 A or 3% T. An absorbance value of 1.5 using the SmartPath 0.02 mm pathlength is equivalent to a 1 cm pathlength absorbance value of 750.

## Beer-Lambert Law

---

The Beer–Lambert Law (or Beer’s Law) combines separate concepts that were first described by August Beer<sup>[1]</sup> and JoHann Lambert<sup>[2]</sup> (Equation 3). Beer’s Law stated that absorbance is proportional to the concentration of the sample. Lambert’s Law stated that absorbance is directly proportional to the thickness (or pathlength) of the sample. The combined law correlates the absorbance to both the concentration as well as the thickness (pathlength) of the sample<sup>[3]</sup> and is generally written as:

$$\text{eq 3: } A = \epsilon bc$$

**A:** absorbance

**$\epsilon$ :** absorptivity coefficient with units of L /mol\*cm

**b:** pathlength of the sample expressed in terms of cm.

**c:** concentration of the sample in solution, expressed in mol/L.

**Note:** 1 cm = 10 mm. All references to pathlengths used on the DeNovix DS-11 and DS-11+ are expressed in terms of mm.

## Absorbance vs. Pathlength

---

As mentioned above, there is a linear relationship between the the absorbance of a sample and the distance (pathlength) that the light travels through the sample. Using shorter pathlengths enables samples with higher absorbances (when expressed as 10 mm equivalent values) to be accurately measured.

The DS-11 uses real-time absorbance data to determine the optimal pathlength for each sample. If a sample absorbance detected at the 0.5 mm microvolume pathlength is too high, the DS-11 software will automatically move the arm down as needed to ensure that the measurement stays within the optimal detection range of the instrument.

The DS-11 microvolume mode uses pathlengths ranging from 0.5 mm down to 0.02 mm. Even when the remarkably short pathlength is used, the typical CV associated with the very high concentrated samples is within 3%.

## Short Pathlengths, High Concentrations

---

The DS-11 software uses the Beer-Lambert equation to calculate concentrations based on absorbance values at specific analysis wavelengths. Keeping in mind the relationships between absorbance, pathlength and concentration described by Beer’s Law, it is easy to understand that a decrease in pathlength (b) permits a corresponding increase in the measurable concentration (c). Figure 2 highlights the maximum concentration for two commonly measured biomolecules using the DS-11 microvolume mode as compared to a traditional 10 mm cuvette based system.

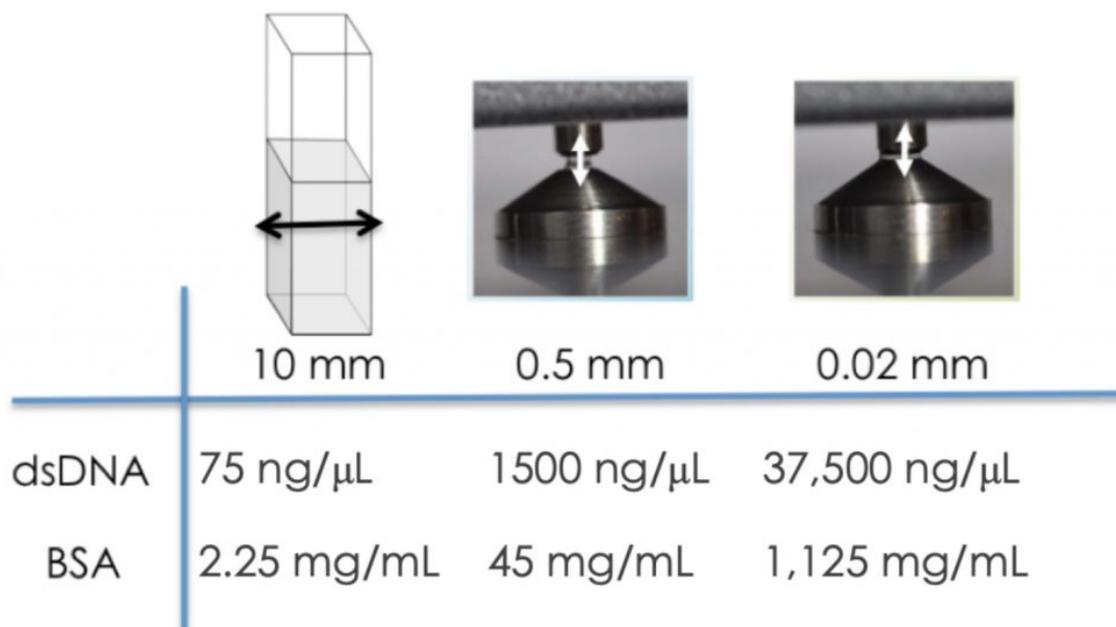


Figure 2: Maximum Concentration as a Function of Pathlength; Abs = 1.5 AU

## Summary

SmartPath Technology enables the DS-11 to measure samples more concentrated than any other spectrophotometer on the market today, making it the ideal choice life science research and manufacturing laboratories.

## References

1. Beer (1852) "Bestimmung der Absorption des rothen Lichts in farbigen Flüssigkeiten" (Determination of the absorption of red light in colored liquids), Annalen der Physik und Chemie, vol. 86, pp. 78–88.
2. J.H. Lambert, Photometria sive de mensura et gradibus luminis, colorum et umbrae [Photometry, or, On the measure and gradations of light, colors, and shade] (Augsburg ("Augusta Vindelicorum"), Germany: Eberhardt Klett, 1760). p. 391.
3. Tissue, B. 2013. Basics of Analytical Chemistry and Chemical Equilibria John Wiley & Sons. Retrieved from <http://books.google.com>.

Revised 19 Oct 2020

DeNovix Inc.  
3411 Silverside Road  
Wilmington, DE 19810, USA

Phone: +1.302-442-6911  
Email: [info@denovix.com](mailto:info@denovix.com)  
[www.denovix.com](http://www.denovix.com)

DeNovix<sup>®</sup>